(54) Title: URETHRAL INSERTED APPLICATOR FOR PROSTATE HYPERTHERMIA

(57) Abstract

A urethral insertable applicator for prostate hyperthermia includes an energy applicator (14) in association with a multi-tube, balloon-type catheter (18). The energy applicator (14) may be a microwave applicator or an ultrasound applicator, either of which, when inserted in the prostate, will cause heating of the prostate tissue surrounding the applicator. The applicator (14), with a radiometer (11), may serve as a means to measure temperature by measuring the thermal energy radiated from the prostate tissue. Provision may be made for circulating a cooling fluid through a cooling chamber (73) between the applicator (14) and the tissue to be heated. The difference in temperature of the inlet and outlet cooling fluid may also be used to indicate prostate tissue temperature. A measure of the temperature of the prostate tissue being heated is used to control application of energy to the applicator.
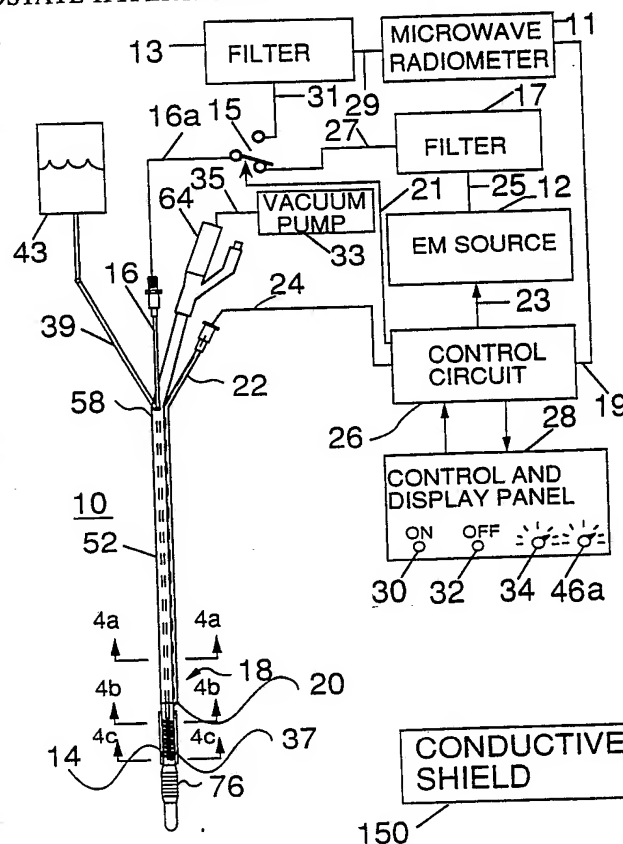
+ DESIGNATIONS OF "SU"

Any designation of "SU" has effect in the Russian Federation. It is not yet known whether any such designation has effect in other States of the former Soviet Union.

FOR THE PURPOSES OF INFORMATION ONLY

Codes used to identify States party to the PCT on the front pages of pamphlets publishing international applications under the PCT.

AT	Austria	ES	Spain	MG	Madagascar
AU	Australia	FI	Finland	ML	Mali
BB	Barbados	FR	France	MN	Mongolia
BE	Belgium	GA	Gabon	MR	Mauritania
BF	Burkina Faso	GB	United Kingdom	MW	Malawi
BG	Bulgaria	GN	Guinea	NL	Netherlands
BJ	Benin	GR	Greece	NO	Norway
BR	Brazil	HU	Hungary	PL	Poland
CA	Canada	IT	Italy	RO	Romania
CF	Central African Republic	JP	Japan	SD	Sudan
CG	Congo	KP	Democratic People's Republic of Korea	SE	Sweden
CH	Switzerland			SN	Senegal
CI	Côte d'Ivoire	KR	Republic of Korea	SU+	Soviet Union
CM	Cameroon	LI	Liechtenstein	TD	Chad
CS	Czechoslovakia	LK	Sri Lanka	TG	Togo
DE	Germany	LU	Luxembourg	US	United States of America
DK	Denmark	MC	Monaco		

1

URETHRAL INSERTED APPLICATOR FOR PROSTATE HYPERTHERMIA

Background of the Invention

Field: This invention relates to energy radiation
devices for medical hyperthermic purposes, and more
particularly to a combined catheter, and energy applicator
for treating prostatomegaly such as benign prostatic
hypertrophy, prostatitis, and prostate malignancy by
urethral insertion.

State of the Art: Hyperthermia or induced high body
temperature has been considered beneficial in treating
various human diseases including many types of cancer.
More specifically, various types of malignant growths are
considered by many researchers to have a relatively narrow
hyperthermia treatment temperature range.   Below a
threshold temperature of about 41.5 degrees Celsius,
thermal destruction of these malignancies is not possible,
and in fact their growth may be stimulated.   However, at
temperatures above a range of about 43 to 45 degrees
Celsius thermal damage to most normal body tissue cells
occurs if exposure lasts for even a relatively short
duration.

Many types of superficial cancers are known to
respond to direct application of surface heat.   Deeply
located malignant growths are most difficult to heat to
the desired temperature without damaging overlying healthy
tissue, owing to limited penetration depth of externally
applied energy, tissue blood flow, and heat transfer
properties of the body.   A solution to this problem has
been the development of electromagnetic (EM) or ultrasound
(US) radiation heating devices for inducing hyperthermia.
This   form   of   treatment   is   historically   known   as
"diathermia".   The EM frequency range preferred is that of
the microwave range which is generally defined as that
above 300 MHz, although the lower defined microwave band
extends to 225 MHz.

EM or US radiation heating of subsurface growths from
an exterior surface is ordinarily enabled by configuration

2

and placement of one or more applicators and by appropriate selection of EM or US radiation frequency, phase and intensity. Nevertheless, tissue growths inside of, or in close proximity to, heat sensitive tissue or organs, are much more effectively and safely heated by EM or US radiation irradiating applicators positioned within the body as closely as possible to the growth requiring treatment.

The advantages of positioning EM or US radiation applicators relatively close to the growth to be heated by radiation include improved heating control, more localized heating, less possibility of overheating adjacent healthy tissue, and more direct treatment of the enlarged tissues causing the undesirable symptoms.

Close applicator access to certain types of diseased tissue growth is provided by surgical procedures for naturally occurring body passages such as the esophagus, larynx, prostate gland and colon. Surgical procedures enlarge the passage by cutting away the diseased tissue. Some heating methods involve placing small EM radiation applicators over the tissue or in an incision to provide direct irradiation of the growth. An illustrative type of a body passage insertable EM radiation applicator is described in United States Patent No. 2,407,690 issued to Southworth. The Southworth type body passage EM applicators have been configured to cause a heating pattern that tends to be concentrated at the radiating tip of the applicator and which decreases at a usually exponential rate from the radiating or distal tip towards the proximal end of the applicator toward the power supply.

Special and difficult problems often attend growths found along natural body passages. For example, diseased tissue tends to spread around and along the passage, often in a relatively thin layer. Typically, the patient problems are confined to originate from a tissue layer which is less than one centimeter thick, and may extend as far as 6-10 centimeters along the passage. The use of

3

Southworth type applicators result in nonuniform irradiation heating of the elongated growth. Thus, the temperature at the distal tip of a Southworth type applicator may have to be so hot that it kills surrounding healthy tissue in order to make the proximal end hot enough to kill the unwanted tissues in that zone.

Rectally inserted rigid and non-flexible antenna devices have been designed for heating of the prostate. Examples of such devices are disclosed in U. S. Patent No. 4,601,296 issued to Yerushalmi, and a 1980 article titled "Microwave Applicators for Localized Hyperthermia Treatment of Cancer of the Prostate," by Mendecki et al., Int. J. Radiation Oncology, Biol. Phys., Vol. 6, pp. 1583 and 1588.

Yerushalmi, et al., published an article entitled "Localized Deep Microwave Hyperthermia in the Treatment of Poor Operative Risk Patients with Benign Prostatic Hyperplasia". This article described initial efforts to heat prostate cancer which involved a substantial amount of the prostate gland. The objective of the treatment described lead them to utilize a rectal approach. They used cooling within the rectum to moderate the localized heating of the rectal mucosa, since the EM energy specific absorption rate (SAR) was much higher in this area near the applicator than within the central prostate area.

It should be pointed out that the urethra is usually about 2cm from the rectal wall. In Benign Prostatic Hypertrophy (BPH) the urethral obstruction is the primary problem for the patient. It would appear unnecessary to treat only the posterior portion of the prostate with heat to relieve a problem primarily confined to the urethral area in the prostate. The concern by Yerushalmi about possible rectal mucosa damage was valid because he was introducing the heating through the rectum. With the urethral approach, rectal heating is not expected to be high because of the 2cm distance between the urethra and the rectum. Thus, Yerushalmi's use of cooling was to

4

protect the rectal wall from excessive heat damage from the rectal applicator.

Yerushalmi, et al. described their treatments as causing temperatures of 42 to 43 degrees Celsius in the prostate mass. These temperatures were measured by monitoring the urethral temperature. This temperature range was obtained after 10 to 15 minutes of heating. Each treatment session lasted for 1 hour and treatments were separated by 72 hours delivered twice per week. The patients' condition improved after 6 to 8 treatments, and they claimed the optimal total number of treatments was 12 to 15. Very low toxicity was reported in these cases. However, the article points out that "heating of normal tissue in the applicator-prostate mass path is unavoidable, since high power field energies are required in order to reach the prostatic mass."

Scheiblich and Petrowicz published an article in 1982 in the Journal of Microwave Power entitled "Radiofrequency-Induced Hyperthermia in the Prostate". The system described in the article was solely intended for treatment of cancer of the prostate and not BPH. Cancerous tumors of the prostate are usually quite large and involve a substantial portion of the prostate when they are detected. It is well-known that treatment of only a portion of the tumor would not be considered sufficient therapy since the tumor would continue to grow from the untreated portions. This would lead to the same undesirable clinical outcome of uncontrolled tumor growth. Thus, it is important that a cancerous tissue treatment be of the whole volume involved in the malignant growth.

The Scheiblich et al. system described used a rectal approach which included rectal cooling with 2.5 degrees Celsius cooling water contacting the rectal wall to reduce the local rectal heating. They claimed that they first experimented with a small antenna that was inserted into the urethra but not enough power could be delivered into the prostate through the antenna in the urethra. The details of this design were not described so it is not

possible to completely evaluate their claims. The article teaches heating from the remote rectal opening. This allowed a larger diameter antenna and longer diameter water bolus to be used producing a larger heating zone.

Helical coil designs have been used to heat tissues placed within the cylindrical opening of the coil. Such devices are disclosed in U. S. Patent No. 4,527,550 issued July 1985 to Ruggera. This heating device was not inserted into the body. Another known apparatus is a body passage insertable applicator apparatus for EMR systems which includes a urethral inserted probe having a monopole antenna ("Microwave Surgical Treatment of Diseases of Prostate," Harada et al., Urology, December 1985, Vol. XXVI, No. 6, pp. 572-576).

Also known is a helical wound coil applicator having coaxial inner and outer conductors electrically connected at an EMR input end to a conventional coaxial transmission line for transmitting high frequency EMR from a source to the applicator. The applicator coil is attached at one end of the outer conductor segment of the coaxial cable. The inner conductor is electrically connected to the other end of the applicator coil. A dielectric media is disposed between the applicator inner and outer conductors, and the outer conductor and termination end are covered by a dielectric sheath. A uniform, external electric tissue heating field is obtained along the entire length of the applicator radiator by exponentially increasing the thickness of the dielectric sheath over the termination end equal to at least half the outer diameter of the applicator. Those persons skilled in the art, desiring further information concerning this device are referred to U. S. Patent No. 4,658,836 issued April 21, 1987 to Paul F. Turner. This patent also contains a circulating fluid filled membrane separating the microwave applicator from the tissue while inserted in a natural body orifice. When this device is used it becomes difficult to directly and accurately measure the temperature of the heated tissue using a single

6

temperature sensor which is housed inside of the
applicator body or attached to the outer applicator
membrane wall. This is because the detected temperature
is greatly affected by the temperature of the cooling
5   fluid, and further modified with unknown blood flow
effects. Therefore, with current technology, accurate
temperature control of the heated portions of the prostate
gland with an applicator containing both cooling as well
as microwave heating would require measurement with a
10   temperature probe inserted into the prostate tissue. The
microwave heating transmits its energy into the tissues of
the prostate. The cooling using conductive heat transfer
is less capable of affecting temperatures in the deeper
tissues and primarily affects the temperature along the
15   applicator-tissue interface.

The use of inflatable balloon catheters is also well-
known in the existing art as described by H. H. Snyder in
U. S. Patent No. 2,936,761. However, the balloon in this
type of catheter, often called a Foley catheter, is
20   generally used to hold a catheter from coming out of a
body cavity, rather than to position a portion of the
catheter in a body passage. Another catheter device made
for insertion into body passages for the purpose of
measuring the temperature along such body passages was
25   disclosed by Bernard Horn in U. S. Patent No. 4,046,139.
This device uses an inflatable balloon to position a small
temperature sensor against the tissue comprising the body
passage, but not to position the sensor along the passage.

A European Patent application No. 83305653.4 filed 22
30   September, 1983 by Kureha Kagaku Kogyo described a dipole
coaxial applicator embedded in an insertable tube which
has a thin polymer layer surrounding the heating zone of
the microwave applicator which is inflated with
circulating cooling fluid. The described use of the
35   applicator is for the heating of endotract lesions. The
prefix endo refers to "inside", which implies use inside
of body passages. The metal wire temperature sensor
placed on the surface of the fluid circulating membrane

7

would certainly not be able to perform a direct or reliable measurement of the surrounding heated tissue, since the sensor is attached to the coolest point adjacent the applicator, the cooling fluid membrane. It is also known that the linear dipole antenna which he describes doesn't provide uniform heating along length of the antenna, thus the heating would not be very uniform along the body passage. The metal wire sensors have also been shown to modify the heating patterns around the metal wire. This is especially true when the wire is aligned with the microwave radiated electric field as shown in the preferred embodiment of that patent application. It is quite important to assure that prostate treatments are reliable and consistent to provide both safety and effective treatments. To achieve this therapeutic goal, it is important to avoid excessive heating of tissues which might result in patient pain and complications, but, at the same time, adequate temperatures must be obtained for a significant time in the targeted treatment tissues on the prostate gland. A lack of a reliable method to measure the heated prostate tissue temperature surrounding the urethra will result in inconsistent treatment results.

The international patent by Bicher WO 81/03616 describes a microwave antenna for intracavitary insertion. This apparatus contains an inflatable jacket which is filled with air and provided with air circulation tubes to provide some cooling. The air flow would have an effect of cooling the adjacent tissues, but would also result in incorrect temperature measurements of the actual surrounding tissue temperatures from the temperature sensors which are placed along the outer wall of the applicator apparatus.

Recently Diederich and Hynynen described use of a rectally inserted ultrasound array device for the treatment of prostate cancer ("Induction of Hyperthermia Using an Intracavitary Multielement Ultrasonic Applicator", IEEE Trans. on BME, Vol. 36, No. 4, April 1989, pp. 432-438). This article describes several

8

ultrasound cylindrical sleeves along an inserted
applicator body. This array construction is relatively
large in diameter, so it is suitable for insertion into
the rectum, but the construction requirements and
5   application of insertion into the urethra for more local
heating of the benign prostate diseases for the purpose of
urinary function improvement is not taught.

The use of microwave radiometry as a means of
temperature measurement with an inserted heating
10   applicator has been described by Convert. Convert in U.S.
Patent No. 4,312,364 has described the use of an invasive
microwave or electromagnetic wave heating probe which is
also used to receive with a radiometric receiver, a
measure of the thermal noise of the surrounding tissue and
15   deduce therefrom the temperature of these tissues.
Convert further suggests using the deduced temperature
measurement to control the power emitted through a
servocontrol system. The microwave antenna is represented
by Convert as being inserted into the tissues of the body
20   using a sharpened tip, hollow slotted needle. This is
used to pierce the skin and penetrate into the body
tissues by cutting into these tissues. After the antenna
is inserted, the insertion needle can then be removed.
This is called interstitial therapy where the devices are
25   inserted by cutting into the body. This type of antenna
is usually quite small in diameter to avoid the
requirement of cutting a large insertion hole into the
patient's body. Convert also suggests that a different
type of probe may be designed for introduction into the
30   human body by a natural route such as the esophagus. For
this purpose, he suggests use of an ovoid dielectric
sleeve around the antenna with permittivity similar to the
coaxial dielectric, such as silicone. There is no tissue
cooling means suggested or possible with the apparatus of
35   Convert, and there is no positioning method provided for
properly locating such a device at the correct treatment
location. The configuration shown for insertion into the
natural body passages has a solid dielectric sleeve, such

as a silicone material, which would not cool the passage
surface, and, as shown, would not be suitable for
insertion or positioning within the prostatic urethra
passage.

5   Other radiometric temperature measurement apparatus
have been reported, but none are as closely related as the
work reported by Convert, who uses them with an invasive
heating device.

10   Summary of the Invention
           According to the invention, an energy radiation
applicator apparatus for treatment of benign prostatic
hyperplasia and other diseases of the prostate gland
locally involved around the urethra, includes a catheter
15   means for insertion into the urethra, an energy applicator
mounted on the catheter, and a connector means extending
along the catheter from the energy applicator to outside
the body when the catheter is inserted in the urethra.
The connector means is adapted to be connected to a source
20   of energy to be supplied to the applicator to enable the
applicator to radiate energy to the tissue surrounding the
applicator to elevate the temperature of such tissue to a
preselected temperature and to maintain the preselected
temperature during treatment.

25   In a preferred embodiment of the invention, the
apparatus includes a fluid receiving means surrounding the
applicator so as to be positioned between the applicator
and the tissue to be heated, and means for circulating
cooling fluid through the fluid receiving means during
30   heating of the tissue to thereby cool the tissue
immediately adjacent the applicator.   A means for
measuring heated tissue temperature is included so that
the temperature of the tissue can be maintained within a
preset range during treatment, and when cooling is used,
35   preferably takes the form of a radiometer selectively
connected through the connector means to the applicator.
When so connected, the applicator acts as an antenna to
receive energy (thermal noise) transmitted from the heated

10

tissue which is representative of the temperature of the
heated tissue and to send such received energy to the
radiometer for measurement. This detected temperature
information can be used to control the amount of energy
applied to the applicator to regulate the tissue
temperature. When using a radiometer, the applicator is
alternately switched between connection with the energy
source and the radiometer.

The energy applicator may be an electromagnetic (EM)
energy applicator in which case the applicator can take
many known forms, such as a coiled conductor in the
catheter, or may be an ultrasonic (US) energy applicator
in which case the applicator may take the form of a stack
of piezo-electric cylinders in the catheter. The piezo-
electric cylinders convert the EM energy into high
frequency mechanical movement of the material. This high
frequency mechanical movement causes ultrasound radiation
to be sent into the tissues surrounding the applicator to
cause heating of the tissue.

The catheter preferable includes an applicator
positioning means for positioning the applicator in the
prostate gland adjacent the tissue to be heated and for
maintaining the position during treatment. The applicator
is suitably sheathed to provide an external substantially
uniform tissue heating field to be radiated at nearly all
transverse cross sections along the applicator for
substantially uniform tissue heating.

A principal feature distinguishing the present
invention from the prior art devices is the provision of
a urethral insertable EM or US radiation applicator,
system, and method principally adapted for benign
prostatic hyperplasia (BPH), which provides the generally
cylindrical or longitudinally uniform EM or US radiation
heating pattern necessary to enable substantially uniform
heating of BPH growths or other tissue diseases associated
with the urinary track, by the combined use of circulating
cooling fluid inside the applicator and monitoring the
heated prostatic tissue temperature by using microwave

radiometry. The unique use of microwave or US radiation
radiometry with cooling in a microwave or US radiation
applicator for the treatment of the prostate has a
specific therapeutic advantage not obtained by other
5   methods and systems. This method is capable of greatly
improving the therapeutic effect from even one treatment.
The hyperthermia treatments with other systems which use
an applicator inserted into the urethra do not contain
fluid circulation cooling and microwave or US radiation
10   radiometric temperature measurements. The unique
combination of these methods enable therapeutic heating of
a much larger prostate tissue volume than other methods as
well as a reliable and accurate measurement of the
therapeutic temperature of the heated prostate tissues.
15   It has been observed in treatments not using cooling in
the urethra inserted applicators, that the therapeutic
temperatures are limited to about a 6 mm radial depth from
the inserted applicator wall. As previously indicated,
the tissue layer causing patient problems is usually less
20   than 10 mm in depth, however, in many cases it will be
greater than 6 mm, therefore, the therapeutic temperatures
may not extend completely through the tissue layer to be
heated. In addition, there appears to be the need for
between five and ten one hour treatments at temperatures
25   ranging between 43 to 50° Celsius. These treatments are
delivered once or twice a week. Early results indicate
that there is a greater therapeutic benefit by the
delivery of ten treatments as compared to five. The
present methods, which are without prostate urethra
30   cooling and microwave radiometry for temperature
measurement, cause the greatest tissue temperatures along
the applicator/tissue interface. This is because the
microwave power is more intense nearest the applicator
radiator. This mechanism enables a temperature sensor to
35   be attached to the applicator wall to at least measure the
prostate tissue temperatures along the wall. When the
cooling is added along the applicator wall, the excessive
tissue temperatures are reduced. This enables more power

12

to be introduced to heat a greater volume of tissue to therapeutic levels. Because a larger volume of tissue is heated to a therapeutic level in each treatment, the need for repeated treatments is decreased.

It has been shown in cancer hyperthermia, that when the target tissues have been adequately treated even one or two times, they will completely respond. The response is normally measured by tissue necrosis. These necrotic or dead tissues are normally absorbed and digested by the natural body process of removing dead cells. Thus, adequate treatment of the tissues within the prostate by even one good heat treatment of the entire target mass is expected to result in the full effect of therapy. This could reduce the number of required treatments from about ten to only one or two. This could greatly reduce treatment costs and inconvenience.

The current methods using microwave urethra heating without cooling have been found to treat to a depth of about 0.6 cm and a length of about 4.5 cm. This results in a treated volume of about 9 cm^3 for a mass of 9 grams. The most common surgical procedure to correct this urinary blockage or retention and other symptoms of benign prostate diseases is the trans-urethral resection of the prostate (TURP). The TURP procedure normally involves the surgical removal of about 15 to 20 grams of prostate tissue along the urethra passage inside the length of the prostate gland. Thus, less tissue is treated by the heat treatment of the first session, than is surgically removed to resolve the symptoms. After the first treatment with current methods, some of the prostate tissues become necrotic and begin to recede by the body's removal of the dead cells. By the next heat treatment several days later, some of the original tissue is most likely not present. This enables a second heat treatment to adequately heat tissues which were beyond the heating depth of the first treatment. Thus, repeated heating treatments are required to eventually treat sufficient tissues to obtain the therapeutic effect and benefit as is

13

provided by the surgical method of (TURP). By using the circulating fluid cooling within the urethra during microwave treatment, the depth of the therapeutic heating is increased because more power can be radiated without

5   causing excessive temperatures. Excessive temperature would certainly contribute to power limiting pain, and may contribute to undesirable toxicity. The volume of tissue which can therefore be treated to therapeutic temperature levels in the first treatment is about 22 cm^3, which is a

10   mass of 22 grams of tissue. This is slightly over that normally resected by a TURP. Thus, the method of cooling within the prostate urethra enables the complete target tissue mass along the prostate urethra to be adequately heated in just one heating session.

15   To provide for a repeatable and safe therapy, it is important to provide sufficient power to reach these therapeutic levels and maintain these temperatures for typically about 60 minutes. Higher temperatures would enable shorter times, but patient pain may prevent

20   temperatures in excess of about 48° Celsius. It is possible to incorporate temperature sensors in the applicator to attempt to estimate tissue temperature, but this would also require monitoring to the radiated power and require performing occasional tissue cool-down

25   measurements to estimate the effect of blood flow, tissue thermal conduction, and bolus cooling effects. This is not expected to be as reliable in all patients as compared with a direct temperature measurement. The preferred method to measure the prostate tissue temperature is by

30   using the heating applicator in a receive mode to direct the thermal noise in the heated prostate region into a microwave or US radiometer. The temperature measurements of the radiometer provide a measurement which is directly related to the temperature within the prostate tissue

35   volume corresponding to the heating volume. This measurement is comprised of adding the temperature signals from the various tissue cells within the applicator's heating field. Therefore, this measurement is like having

14

thousands of individual temperature points which are measured and then added together to provide an indication of the average temperatures within the heated region. This method does not measure the maximum or the minimum temperature in the heated tissue, but provides an accurate measure of the average tissue temperature within the treatment zone. This new method enables the treatment of benign prostate disease to be efficiently treated with hyperthermia, where the tissue being treated is the same tissue which would have been surgically removed by a TURP.

In many patients there are severe side effects by the TURP procedure such as incontinence, retrograde ejaculation, impotency, and death. It is estimated that between 0.3 to 3% of the patients receiving the TURP surgical procedure die from either the procedure or by other factors related to the procedure. Many patients are poor surgical risks due to their age and poor health. The use of hyperthermia treatments as described herein, represent a non-surgical alternative therapy for the benign prostate disease. The optimal combined utilization of the urethra inserted radiating energy microwave source, the circulation cooling fluid in the urethra, the positioning and urine drainage system of the Foley catheter, and the microwave radiometry provides a very practical method to treat benign prostate disease. It is also feasible that this method will be suitable for the treatment of malignant prostate disease. The malignant prostate disease normally involves a larger size mass requiring treatment than is possible with the urethra inserted applicators. However, the increased treatment volume provided by this new method may enable some malignant prostate tumors to be effectively treated as long as the tumor resides within the therapeutic heating area which extends to about 0.8 cm away from the inserted applicator wall. Certainly if the urethral blockage through the prostate is caused by malignant growth, the use of this method to relieve the blockage symptom is also feasible, even though the intent would possibly not be to

cure the cancer if the cancerous growth was larger than the heating volume.

The use of ultrasound crystal cylinders is also considered feasible with this method which can operate as both energy transmitters as well as ultrasound radiometric temperature sensors. In this form, the ultrasonic thermal energy radiated by the tissue within the ultrasound applicator's heating zone will be detected by the ultrasound radiometer. This would therefore be equivalent to the microwave urethral inserted applicator, but would operate at ultrasound frequencies. Various ultrasound cylinders are commonly available such as from the EBL Company of Hartford, Conn. It is preferred that a longitudinal stack of ultrasound crystals be used to enable more flexibility and bending of the inserted crystals.

During radiometry measurements, it is possible that EM noise sources other than the heated tissue, such as fluorescent lights, radio stations, microwave ovens, etc., can interfere with the accurate operation of the EM radiometer. It is possible to perform the application of this EM method inside a metallic shielded room to block out many EM sources which would otherwise possibly interfere with the EM radiometry operation. The addition of a shielded room facility to improve the operation of a radiometer is not considered novel, but is well-known in the current application of radiometry. However, where a shielded room is not available, or where other EM sources may be located in the shielded room, it is useful to include an electrically conductive shield or blanket over or around the patient in the treatment area to reduce the effects of these other EM noise sources on the radiometer. Suitable materials for this shielding blanket are metal screen or mesh, such as that produced by Cleveland Wire Cloth Manufacturing Company of Cleveland, Ohio. The conductive sheet may be in the form of a metal impregnated paper such as that produced by Zippertubing Company of Los Angeles, CA, or by International Paper of Tuxedo, NY. The

16

conductive sheet may even be a metal foil sheet which is commonly marketed as aluminum foil. A practical other shielding material is conductive cloth such as that manufactured by Devex S.A. of Denis, Switzerland, or the Hexcel Corporation of Dublin, California. It is best that these sheets be connected (or grounded) to the outer conductor of the interconnecting applicator cable 16 shown in the Figures.

Advantages of the present invention is the provision of a low cost, disposable applicator which is an integral part of a modified balloon type Foley catheter for the treatment of BPH. BPH is usually treated by surgery with significant side effects. These side effects include hemorrhage, impotency, anesthetic complications, and technical failures. The use of the combined applicator catheter apparatus involves a treatment which requires no anesthesia or surgery and requires only 1 or 2 hour office visits to accomplish in comparison to post surgical hospitalization. The improvements of using the urethra cooling and the radiometric temperature measurement may enable a single treatment to be adequate to provide sufficient symptomatic relief as compared to the need of many treatments each a few days apart when the cooling is not used.

Brief Description of the Drawings

Other objects and features of the invention will become more readily apparent from the following detailed description when read in conjunction with the accompanying drawings, in which:

FIGURE 1 is a view of the urethral insertable EM applicator system showing the schematic diagram in block form;

FIGURE 2 is a functional schematic view of the temperature sensor and EM source control functional circuits.

FIGURE 3 is an exploded view of the urethral insertable EM applicator;

FIGURE 4 contains three cross sectional views, 4a, 4b, and 4c, of the urethral insertable EM and US applicator assembly; taken on the lines 4a-4a, 4b-4b, and 4c-4c of Figure 1.

FIGURE 5 is a view showing the SAR distribution of the EM prostate applicator measured in prostate tissue equivalent phantom tissue.

FIGURE 6 is a longitudinal section of an EM prostate applicator showing the antenna coil radiating configuration.

FIGURE 7 is a functional block diagram of a Dicke Switch style of radiometer for measurement of tissue radiated thermal noise.

FIGURE 8 is a view of the urethral insertable US applicator system showing the schematic diagram in block form.

FIGURE 9 is an exploded view of the urethral insertable US applicator.

FIGURE 10 is a view of the ultrasound radiating transducer cylindrical crystals and their series interconnection.

FIGURE 11 is a view of an alternate series connection configuration for the ultrasound radiating transducer crystals.

FIGURE 12 is a view of an alternate urethral insertable EM applicator system incorporating cooling fluid temperature measurements to determine tissue temperature.

FIGURE 13 is a longitudinal section of an EM prostate applicator similar to Figure 6, but showing the opposite side of the catheter with the fluid drainage passage.

Detailed Description of a Preferred Embodiment

Referring now to Figure 1, the urethral insertable electromagnetic (EM) radiation applicator system 10 includes an electromagnetic energy source 12 having an oscillator for supplying a maximum 40 watts electrical power at a microwave frequency (typically between 300 to

2450 MHz frequency), for example, to an antenna or applicator 14 through a connector means in the form of a connector cable 16 extending through a catheter 18 from antenna 14 to outside the catheter, and a coaxial cable 16a connected to the end of connector 16. A suitable cable for both the connector cable 16 and coaxial cable 16a is a typical RG-178B cable or one of equivalent size. The antenna 14 is a microwave helical coil mounted in the catheter 18 with the end farthest from the power source 12 preferably soldered to the tip of the solid inner conductor of connector cable 16 and the end closest to the power source preferably soldered to the outer braided conductor of the connector cable 16. The catheter 18 is, for example, a size fourteen French catheter modified as hereinafter described.

The coil of antenna 14 may contain one or more of the following physical features:

    a)   open connection between the tip of the coil and center coaxial conductor;

    b)   open connection to the base of the coil and the outer coaxial conductor;

    c)   conductor breaks or gaps within the coil winding;

    d)   multiple-wrapped coils co-located at the same zone

    e)   multiple coils stacked longitudinally and connected to individual coaxial cables to allow modification of the heat pattern length using either coherent or non-coherent phase energy into each coil;

    f)   flexible straight conductors rather than coiled conductors;

    g)   a coil with progressively increasing or varying conductor width towards one end of the applicator;

    h)   a coil with different turns ratio per unit length;

    i)   diameter variations of the center conductor within the coil length; and

j)   modification of the dielectric material or thickness around the center conductor or coil antenna.

A separable insulated temperature sensor 20, Figure 2, located at the tip of insertable lead 24, is inserted in a flexible tube 22, Figure 1, during treatment to provide monitoring of tissue temperatures along the length of catheter 18. The insertion depth of the sensor 20 is manually changed within catheter tube 22 to obtain temperature readings along the length of catheter 18. The tube 22 is attached exteriorly of the catheter 18 and the tip of tube 22 extends almost to antenna 14. The temperature sensor measures the temperature of the urethra tissue surrounding the catheter not located in the prostate. The temperature sensor is connected by an insulated four resistive lead cable 24 to a temperature sensor circuit in control circuit 26 for display and recording functions. The temperature sensor circuit includes a constant current source 38 to provide current to the temperature sensor 20 which is preferably a precalibrated thermistor. An amplifier 40 is connected to the thermistor 20 for amplifying the thermistor output to a working level. While the output of amplifier 40 could be used for control purposes as shown in our patent application, in the illustrated embodiment, the output will usually be connected to a display and used only for information purposes.

A microwave radiometer 11 is connected by cable 29 to an input band pass filter 13 which is connected to a remotely operated function switch 15 with coaxial cable 31. This function switch 15 operates to select either the EM heating mode or the radiometric temperature measurement mode. When switch 15 is in the radiometric mode, the switch connects the microwave radiometer 11 and filter 13 to the applicator coil 14 via the connector cable 16 and coaxial cable 16a. In this mode the thermal energy emitted by the warmed prostate tissue is received by the applicator coil 14 acting as an antenna. This energy is then directed via connector cable 16 and coaxial cable 16a

20

through switch 15 and cable 31, into the filter 13, and through cable 29 to radiometer 11 for detection.   The output of radiometer 11 is directed through cable 19 to the control circuit 26 which is used to regulate the

5   tissue temperature by controlling the output power of the EM source 12.

When the switch 15 is in the heating mode of oepration, as shown in Figure 1, the applicator 14 and cables 16 and 16a are connected through cable 27 to the

10   filter 17 and from filter 17, through cable 25, to the EM source 12, whereby the power generated by EM source 12 is directed to applicator 14 and is radiated into the surrounding tissue by the EM applicator 14. The selection of the heating mode or the radiometric temperature

15   measurement mode is controlled by a signal from control circuit 26 through line 21 which is connected between switch 15 and system control circuit 26. Control circuit 26 controls the level of output radiated power from the EM source 12 and is connected to EM source 12 by cable 23.

20   The control circuit 26 has its output connected to the EM source 12 for controlling the EM power source so that it puts out sufficient power to maintain a tissue temperature between about 41.5 degree Celsius to about 47 degree Celsius. A control and display panel 28 is connected to

25   the control circuit 26 for two way communication. The control and display panel 28 includes EM radiation energy on/off switch buttons 30 and 32, and a temperature controller knob 34 for setting the desired operating temperature for the apparatus.

30   Figure 1 also shows an elevated sterile water-filled chamber or cooling fluid reservoir 43 connected by a tube 39 to a cooling fluid inlet passage 59, Figure 4, to enable cooling water to flow through a fluid inlet to inflate and flow through a fluid receiving means in the

35   form of a thin-walled flexible rubber or plastic cylindrical bolus sleeve 37 which surrounds the radiating applicator 14 to cool the prostate tissues. The fluid filling this bolus 37 is allowed to flow through a small

orifice or fluid outlet in the catheter wall into the urine drainage passage. This urine drainage passage acts as a cooling fluid outlet passage and is connected to a drainage connector 64 to enable these fluids to leave the

5 body. To aid in the urine and fluid drainage, the drainage tube connector 64 may be connected to a vacuum pump and storage chamber 33 by a tube 35. In this way, cool fluid stored in the chamber 43 is caused to flow into the bolus 37 inflating the bolus with water, and fluid in

10 the bolus flows out of the body through the connector 64, assisted by the vacuum created by the vacuum pump 33. Vacuum pump 33 preferably includes a fluid storage chamber for receiving and storing the removed waste fluids. It is necessary that the chamber 43 be adequately elevated to

15 inflate the bolus 37. It may be necessary for the chamber 43 to contain a regulated positive pressure pump to assure that adequate inflation of the bolus membrane 37 occurs. This fluid flow provides cooling of the prostate tissues adjacent to the applicator 14 and inserted catheter 18.

20 Also, the fluid flow along the input tube 39 flows adjacent to the applicator internal connection cable 16 to provide some regulation of the cable temperature to reduce the effect of the cable temperature on the radiometric thermal detection level.

25 The microwave radiometer 11 is connected to the control circuit 26, Figure 1, to direct the radiometric temperature measurement to the control circuit. This enables the control circuit to modify or modulate the EM power output of the EM source 12 to control the tissue

30 temperature to that desired as detected by the microwave radiometer 11. Figure 2 shows that an amplifier 42 is connected to the radiometer output for amplifying the microwave radiometer output signal level. This amplifier function may be incorporated into the radiometer as well.

35 Internal to the microwave radiometer the detected signal must be amplified and integrated (averaged) for about one or two seconds to obtain an accurate measure of the radiometer output. The amplifier 42 also acts as a signal

level comparator and has its second input terminal connected to a temperature setting potentiometer 44 which is connected to or controlled by the temperature controller knob 34 located on the control and display panel 28, Figure 1. Amplifier 42 compares the output of radiometer 11 with a desired temperature reference voltage from potentiometer 44 as set by the temperature control knob 34, Figure 1, and outputs a temperature difference signal to EM source control signal switch 48. The amplifier 42, Figure 2, has its output connected to the junction of a timer 46 and an electrically controlled pole of the double pole switch 48. Switch 48 is controlled by the control panel ON switch 30 and OFF switch 32 which enables treatment to proceed. If the ON mode has been selected and the timer 46 has been set by means of knob 46a on control panel 28 to something other than 0 minutes, the output of the comparator 42 will be directed to the EM source 12 by output signal cable 23. If the timer 46 reaches 0 minutes, the output signal of the comparator 42 is prevented from passing to the EM source by being connected to ground in the timer. This prevents microwave output power from the EM source and stops the heating process. The position of switch 48 is shown connecting the output of comparator 42 to the EM source connecting cable 23, which is the position for the ON mode. Also, in this position, current flows through indicator lamp 50 to indicate ON condition. If timer 46 grounds the signal to stop the heating process, lamp 50 will go out. If the OFF mode is selected by control panel switch 32, the switch position of switch 48 is changed and directs the signal to ground through an indicator lamp 51.

A conductive shield 150 in the form of a sheet or enclosure may be placed over the patient's treatment area or wrapped about the treatment area to reduce the stray electromagnetic noise which may be picked up by the radiometer from other noise sources. These stray signals may degrade the accuracy of the radiometric temperature measurement.

The timer 46, Figure 2, is triggered by the initial receipt of power from the comparator 42 for measuring a preselected treatment time, and at the end of the timing period cuts off the microwave power source. In addition, the pole of the switch 48 is manually controlled by the ON and OFF switch buttons 30 and 32. When the switch is positioned ON as shown, a control signal is output on lead 23 to power the EM power source; conversely, when the switch 48 is turned to the OFF position, the EM radiation power source is turned off. It should be noted the timer 46, comparator 42, temperature setting 44, control switch 48, and other portions of the control circuit can be replaced by a small computer chip such as a microprocessor, operating in an equivalent manner. The use of a small microprocessor performing these represented functions is actually the preferred embodiment of the control system.

The catheter 18, Figure 1, of the combined catheter and applicator is, for example, a balloon-type urological catheter having a flexible, plastic tubular body 52, Figures 3, 4a, 4b, and 4c, which is divided by a partition 54, Figure 4a, 4b, and 4c, into a catheter drainage passage 56, a passage 59, and a fluid passage 60 for inflating balloon 76, Figure 3. The flexible tube 22, Figure 4a, for the temperature sensor is attached to the exterior end of the Foley catheter body 52. The tubular body 52 has a bifurcated opening piece 62, Figure 3, having one side 64 for connecting the central drainage tube 56 to a waste receiving receptacle or vacuum pump, and a second side 66 having an air or fluid input/output valve 68 for connecting the air or fluid passage 60, Figure 4a, 4b, and 4c, to a pressurized air or fluid supply source to inflate the balloon 76, Figures 1 and 3 after insertion. This air or fluid supply source could simply be a syringe.

The coaxial connector cable 16 with an insulating rubber jacket 58 passes through the hole 57 into catheter passage 59, Fig 4a. The insulated coaxial cable passes

24

along the inner chamber and connects to the antenna coil 14 as previously described. If cooling fluid is to be circulated through the catheter, catheter passage 59 becomes a cooling fluid inlet passage and will have cooling fluid flowing therein. The coaxial insulating jacket 58 will be sealed in the areas of connection to the antenna 14 to prevent contact with the water or other cooling fluid which will fill this passage 59. The passage 59 is normally connected through hole 61 with an attached tube 63 and connector 65 to the water fluid supply tube 39, Figure 1. The holes 57 and 61 both lead into the passage 59, so that the coaxial cable 16 rests within and extends along passage 59 in catheter body 18. A pair of openings 79, Figures 4c and 6, are provided through catheter wall 52 into passage 59 adjacent to the distal end of applicator 14, which forms a fluid inlet to allow fluid to flow into and partially inflate a fluid receiving area, or chamber 72, Figure 4b and 4c, formed by a cylindrical bolus membrane 71, which presses against the tissue walls and separates the membrane 71 from the antenna 14 and its dielectric coating tube 70. This fluid filling the receiving area 71 is allowed to flow through a fluid outlet 56a, Figure 46 and 13, into the inner fluid drainage passage 56 which is connected between the tip hole 75 and the drainage connector 64. Fluid drainage passage also serves as a urine drainage tube with tip hole 75 opening into the patient's bladder during treatment.

The dielectric coating tube 70 of, for example, silicone rubber, is placed and bonded over the spiral metal coil 14 to complete the applicator. The dielectric coating or sheath 70 is the means for causing the external, electric tissue heating field to be substantially uniform along the length of the applicator. The thickness of the sheath may be varied exponentially if necessary to obtain the uniform heating field. An additional flexible silicone or plastic tube 71 is also placed over the applicator coil 14 and sleeve 70, and bonded at both ends. This enables water to be inserted

into the water bolus tube compartment created by the bonded outer sleeve 71. The tip zone inflatable balloon 76 is used to position the applicator body properly within the prostate gland. This balloon 76 is inflated with

5   water or air by the self-sealing valve 68, Figure 3, which is connected by a small connecting tube 60 in the catheter wall 52. The catheter is inserted into the urethra a distance so that balloon 76 is inserted into the bladder prior to being inflated. Balloon 76 is then inflated and

10 pulled back to rest against the bladder neck. The positioning balloon 76 is formed by bonding the cylindrical balloon tubular form at its ends to the catheter body 58 at locations 72 and 74. Thus, the inflatable positioning balloon 76 is positioned between

15 the balloon bonded stops 72 and 74 in open communication with the outlet of the air or fluid passage 60 (Figures 4a, 4b, and 4c). Thus, when the catheter is positioned so that the inflated balloon is resting against the neck of the bladder, the applicator is properly positioned with

20 respect to the prostate gland and free from movement for the duration of the hyperthermic treatment.

In operation, with the catheter properly positioned as described above, and the timer 46 of Figure 2 and the temperature dial set as desired, the EM source 12 of

25 Figure 1 is turned on by switch 30 and the applicator 14 radiates power into the area of the prostate gland until the desired temperature is reached. When the desired temperature is reached, the comparator 42 outputs control signals to the oscillator to manipulate its EM radiation

30 output power to maintain the radiometric temperature substantially constant for the selected treatment time period. At the end of the treatment time, the EM source is automatically turned off, but the EM source can be turned off at any time using the off switch 32. During

35 the heating period the control circuit actually interrupts the connection of the EM source power through switch 15 to applicator 14 periodically for a few seconds at a time and connects applicator 14 through mode switch 15 to the

26

radiometer to update the measurement of tissue temperature.

Figures 4a, 4b, and 4c show the cross-sectional views taken on the lines 4a-4a, 4b-4b, and 4c-4c, respectively, of Figure 1. Figure 4a shows the section comprising the major portion of the length of the catheter 18. Passage 60 connects to tip balloon 76. Cooling fluid inlet passage 59 supplies cooling fluid from reservoir 43, Figure 1, to cooling fluid receiving area 73 shown in Figures 4b and 4c. The coaxial connector cable 16 is routed through the fluid inlet passage 59, and includes a center conductor 16d and an outer conductor 16b, separated by a dielectric 16c. Passage 56 is a fluid drainage passage and also serves as the cooling fluid outlet passage. Passages 59 and 56 are separated by a partition 54. Also shown is the outer attached tube 22 through which the secondary temperature sensor 20 passes to monitor urethra temperature.

Figure 4b is taken through the zone of the antenna radiating helical coil applicator 14. Between the views 4a and 4b, the outer conductor 16b of connector conductor 16 has been electrically connected to the proximal end of the antenna coil 14 by passing through the catheter wall 52 and the insulating coating 58. This electrical connection must be sealed from the cooling fluids in passage 59 with a dielectric material such as silicone rubber adhesive. Therefore, in Figure 4b the outer conductor 16b is not seen and the cross-section of the helical conductor strip 14 can be seen. The outer sheath dielectric layer 70 is also seen overlying the conductor 14 and the catheter body 52. Normally the space between the sheath 70 and the catheter body 52 is filled with silicone sealant or adhesive. The flexible outer cylindrical bolus sleeve 71 is also shown forming the outer shell. The fluid receiving chamber 73 between sleeve 71 and sheath 70 is normally filled with a cooling fluid such as water which is supplied by the water storage

reservoir 43, Figure 1, or by some other source of cooling fluid.

Figure 4c is taken through the zone of the distal connection to the helical coil 14 with the center conductor 16d. This connection is provided by an interconnecting wire 80 and soldering with biocompatible solder. It is not advisable to use lead-based solder for such an inserted device, but tin and silver solder is suitable. The fluid outlet opening 56a is used to interconnect the cooling fluid chamber 73 to the fluid drainage passage 56. In this way the circulating cooling water may continue to flow through the fluid chamber 73 which is able to provide substantial tissue cooling through the contacting outer sleeve 71.

The apparatus was tested using muscle equivalent phantom material having a relative dielectric = 69.0 and conductivity = 1.446 mho/m to simulate prostate tissues and the Iso-SAR (specific-absorption-rate) distribution curves charted as shown in Figure 5. The test parameters were as follows:

> Frequency = 915 MHz
> SAR @ 100% = 115.8 W/Kg
> Forward power = 20 Watts
> Reflected power = 2 Watts
> Heat-up time = 30 Sec.

As shown in Figure 5, the measurement boundaries were 10 cm. in the x direction and 0 to 1.5 cm to the sides of the applicator body in the y direction. The SAR gradient was 200% down to 20%. The rate of initial temperature rise is proportional with these SAR percentages. Thus, the helical coil type applicator provides a long, uniform, shallow, heat pattern desired for treating diseased tissue found to have spread around and along the body passages.

Figure 6 shows a cross-sectional view along the long axis of the applicator in the region of the antenna 14. The insulated coaxial cable 16 can be seen passing within the catheter body 52. At the proximal end of the coil 14 the outer conductor 16b is connected to the coil 14 with

28

an insulated wire 81. At this point the outer conductor
ends and only the coaxial inner conductor 16d, dielectric
sleeve 16c, and insulating sleeve 58 of the coaxial cable
extend to the distal region of the coil 14. Also shown is
5   the fluid stop 72 for the tip inflatable balloon 76. The
fluid cooling chamber 73 is shown to extend slightly
beyond the zone of the coil 14 at both ends. Attachment
of the outer flexible bolus membrane 71 is attached at
both distal and proximal ends to the catheter body 52 with
10   adhesive such as silicone rubber (not shown). The
dielectric sheath 70 may be tapered in thickness, and
covers the coil 14 with ends 77 sealed with silicone
rubber. The two holes 79 passing through the catheter
body 52 to the distal end of fluid chamber 73 enable fluid
15   to pass from the fluid inlet chamber 59 to the bolus fluid
receiving chamber 73. These holes in combination with the
hole 56a of Figure 4c enable the fluid to flow from
reservoir 43, Figure 1, through the cooling bolus chamber
73, and be discharged through the drainage connection 64,
20   Figure 1, into the vacuum pump storage compartment 33. To
insure inflation and proper filling of fluid receiving
chamber 73, the two inlet holes 79 provide a larger fluid
inlet than the single outlet 56a. With this arrangement,
it is assured that less fluid can flow from the chamber
25   than can enter it so the chamber will remain full of fluid
as long as fluid remains in the fluid supply reservoir.

The design of a conventional Dicke Switch radiometer
is shown in Figure 7. The purpose of such a radiometer is
to enable very accurate measurements of very weak energy
30   signals. The input signal as supplied on line 29 from
filter 13, Figure 1, is connected with a transmission line
83 to the input band pass filter 82. This filter is
recommended to operate with about a 10 MHz bandwidth at a
frequency between 300 to 2450 MHz. The signal is routed
35   to a calibration switch 86 by cable 84 which is normally
a mechanical relay coaxial switch. This switch is changed
between connection to either the input signal or a
constant known temperature resistive load 88. The signal

is then routed through cable 90 to a rapidly switched
microwave switch called a Dicke Switch 92 which is
commonly a solid state switch. The Dicke Switch switches
between the signal level and a resistive load 94 at known
5   constant temperature.   This Dicke Switch is commonly
switched at a rate between 100 to 1000 Hertz driven by the
Switch Driver 114 by interconnect cable 116. The switch
modulated output of the Dicke Switch 92 is routed to a
series of amplifiers 98 and 106 and additional band pass
10   filter 102 with cables 96, 100, and 104. The amplified
and filtered signal is then sent by cable 108 to a diode
detector and filter 110 to eliminate the microwave portion
of the switched signal. The signal is then sent into a
demodulating relay switch 118 by cable 112, where the
15   thermal noise signal originating from the resistive load
94 is directed to an inverting unity gain amplifier 126 by
cable 122, and the filtered and amplified signal from the
input 83 is directed to the non-inverting amplifier of
unity gain 124 by cable 120. These two amplifier outputs
20   are added together by a summer 132 and interconnected by
cables 128 and 130.   The output of the summer 132
represents the dc error voltage signal representing the
difference temperature between the input signal and the
reference load 94 temperature. This signal is directed to
25   an integrator 136 with a few seconds of integration time
by cable 134. The output of the integrator 138 can be
interpreted directly as a temperature difference from the
reference load 94 physical temperature. Many other types
of radiometers are suitable for use with this system as
30   well as the more common Dicke Switch type and should be
considered an equivalent part of the described system.

          Figure 8 is a system diagram similar to that of
Figure 1, but shows the varied components to use an
ultrasound radiator 14 and an ultrasound frequency range
35   radiometer 11 which would operate at a frequency of
between 0.5 to 5 MHz with a bandwidth of between 10 to
1000 kHz. Note that the EM source 12 would also operate

30

at lower EM frequencies between 0.5 to 5 MHz. All other components operate as previously described.

Figure 9 is similar to Figure 3, but shows a stack of ultrasound piezo electric cylinders 14 replacing the microwave coil 14 of Figure 3.

Figure 10 shows a more detailed arrangement of the individual piezo electric cylinder 140 comprising the radiating ultrasound stack 14. The coaxial cable 16 is represented where the center conductor 16d, passed through the center of the stack and is connected at the distal end of the stack 14 with conductor 80. The cylinders 140 are metal plated on both cylindrical surfaces so the attachment of wire 80 to the outer surface of the most distal cylinder 140 can be made with silver and tin solder. The outer conductor is not shown, but would connect to wire 146. Wires 142 and 144 show series connection of the cylinders 140 to comprise a series connected stack each being soldered as shown. Here the central surfaces of the cylinders are connected together with wires 142 and the outer surface of the cylinders are connected with wire 144.

Figure 11 shows an alternate assembly of the ultrasound piezo electric stack 14 where wires 148 are used to interconnect the cylinders 140 in series. Here the central surface of each cylinder proceeding from the distal end is connected to the outer surface of the adjacent cylinder. The function will be the same for either Figure 10 or 11.

It is also a part of this invention to measure the temperature of the input and output water flow of the urethral inserted applicator as well as the water flow rate to predict the amount of heating being imparted to the prostate tissue. This could be used either in combination with the microwave or ultrasound radiometry or could be in place thereof. There is a relationship between the amount of power being removed by the urethral cooling and the temperatures reached within the prostate tissues. More importantly there is a relationship between

the temperature of the cooling water in the inflated water bolus zone and the temperature of the prostate tissues in contact with the urethral applicator. The limitation of tissue temperatures within the tissues forming the lining

5 of the urethral passage, will provide a limitation to the toxicity and patient complications. It is not certain exactly the preferred limitation of these tissues contacting the urethral applicator, but it is expected that this temperature should be limited to below 45°C to

10 avoid excessive damage to these urethral tissues. By adding two additional temperature measurement probes to measure both the input water temperature and the output water temperature the temperature of the urethral tissue in contact with the water bolus can be determined as

15 described below.

The heat transferred from the prostate, through the bolus wall, and into the cooling fluid can be quantified using the mass flow equation, $q = (dm/dt) \, Cp \, (T_{out}-T_{in})$, where "q" is in units of kcal/second. The mass flow rate

20 (dm/dt) is determinable and controllable since it is simply a measure of the rate of water flowing through the water bolus, the specific heat of water (Cp) is known to be 1 kcal/kg °C, and the temperature differential ($T_{out}-T_{in}$ is measurable by locating temperature probes within the

25 applicator body or in the interconnecting tubes. The above enables "q" to be determined from the water flow rate and the measurement of input and output water temperatures. To determine the power "P" which is being removed by the flowing water, the following simple

30 equation is used: $P=1.163q$. To determine the surface temperature of the urethral prostate tissue in contact with the water bolus zone a simple application of the thermal conduction and convection problem can be used which is the equivalent of Ohm's Law, i.e. $[T1-T0]=q \, r$,

35 where "r" is the sum of thermal resistances from the prostate tissue boundary with the applicator, through the bolus wall, and into the cooling fluid. The specific equation is:

32

$$[T1-T0]=q\{[1/A1(k)]+[1/h(AO)]\}, \text{ where,}$$

T1=unknown temperature of tissue

T0=average temperature of cooling water in the bolus, or $[T_{out}=T_{in}]/2$

5   l=thickness of bolus material

k=coefficient of thermal conductivity of bolus material (silicone)

h=coefficient of convection from inside bolus wall into cooling water, determined by calculating the Reynold's number of flow through the bolus channel.

A1=surface area on outside surface of the bolus

AO=surface area on inside surface of the bolus.

So, by controlling and knowing the mass flow rate of the cooling water, and by measuring the temperature rise of the water, the temperature of the prostate surface in contact with the applicator is readily calculated by a system computer or measurable by specialized circuitry to enable the proper amount of power to the tissues to limit the urethra tissue wall temperature to the level below typically 45°C.

In addition, the measure of the forward and reflected microwave or ultrasound power delivered to the applicator as well as the radiating efficiency of the microwave or ultrasound energy radiator can be compared with the amount of power being removed by the water bolus. The power "P" being removed by the bolus can also be used. When adequate clinical information is obtained using prostate tissue measurements with other temperature probes inserted into the prostate, a correlation with the power delivery into the prostate and the power drawn off by the water cooling could be used to directly control the input power for the treatment.

A system incorporating measurement of the inlet and outlet temperatures is shown in Figures 12 and 13. A monitor 156 is provided in cooling fluid supply line 39 to measure the temperature and flow of cooling fluid into catheter 18. While the temperature of the outlet fluid could be measured, since it is mixed with urine draining

33

from the bladder which will affect the temperature, it is preferred to measure the temperature of the outlet cooling fluid at the fluid outlet from chamber 73 before the fluid enters outlet passage 56. For this purpose, a temperature
5   sensor 162 is positioned in fluid receiving chamber 73 adjacent fluid outlet 56a as shown in Figure 13. Resistive leads from temperature sensor 162 extend through a flexible tube 152 secured to catheter 18 similarly to tube 22, and connects to monitor 156. Signals
10   representative of the temperatures and flow of cooling fluid are sent from monitor 156 through cable 158 to microprocessor 160. Microprocessor 160 is programmed to perform the desired calculations as described to provide an output representative of the temperature of the heated
15   tissue. This output from the microprocessor is transmitted through line 19 to the control circuit 26 where it can be used in exactly the same manner as the radiometer signal to control operation of the system as described. In such instances, the microprocessor is
20   substituted for the radiometer in Figure 2. However, both types of measurement could be used in a system with one or the other or both used for control and/or information purposes.

While the temperature sensor leads for sensor 20 and
25   162 have been described as resistive, since the sensors only enter the periphery of the energy fields, the resistive leads may not be necessary and normal wire leads could be used.

Whereas this invention is here illustrated and
30   described with specific reference to embodiments thereof presently contemplated as the best mode of carrying out such invention in actual practice, it is to be understood that various changes may be made in adapting the invention to different embodiments without departing from the
35   broader inventive concepts disclosed herein and comprehended by the claims that follow.

34

Claims

1.   An energy radiation applicator apparatus for
treatment of benign hyperplasia, comprising:

            a catheter means for insertion into the urethra;

            an applicator means attached to the catheter
means, said applicator means including an applicator and
a connector means for connecting the applicator to a
source of energy sufficient to elevate the temperature of
tissue   surrounding   the   applicator   to   a   preselected
temperature   and   for   maintaining   the   preselected
temperature during treatment;

            fluid receiving means surrounding the applicator
so as to be positioned between the applicator and the
tissue to be heated; and

            means for circulating cooling fluid through the
fluid receiving means during heating of the tissue.

2.   An   energy   radiation   applicator   apparatus
according to Claim 1, wherein the means for circulating
cooling fluid through the fluid receiving means includes
a fluid inlet through which cooling fluid is supplied to
the fluid receiving means and a fluid outlet through which
fluid flows from the fluid receiving means, said fluid
inlet and fluid outlet being positioned with respect to
the fluid receiving means so that fluid flowing from the
inlet means to the outlet means will flow substantially
through the fluid receiving means.

3.   An   energy   radiation   applicator   apparatus
according to Claim 2, wherein the catheter means includes
a   cooling   fluid   inlet   passage   extending   through   the
catheter to communicate with the fluid inlet, and a
cooling   fluid   outlet   passage   extending   through   the
catheter to communicate with the fluid outlet, both the
fluid inlet passage and the outlet passage opening from
the catheter outside the body when the catheter is
inserted into the urethra.

4.   An   energy   radiation   applicator   apparatus
according to Claim 3, wherein the outlet opening is
smaller than the inlet opening to cause fluid pressure

build up in the fluid receiving means to thereby insure the presence of fluid in the fluid receiving means when fluid is provided to the fluid inlet.

5. An energy radiation applicator apparatus according to Claim 4, wherein the catheter extends through the urethra into the bladder, and wherein the cooling fluid outlet passage also functions as a urine drainage passage for draining urine from the bladder.

6. An energy radiation applicator apparatus according to Claim 5, wherein the fluid outlet of the fluid receiving means connects to the outlet passage intermediate its length through the catheter.

7. An energy radiation applicator apparatus according to Claim 6, wherein a source of vacuum communicates with the outlet passage opening from the catheter outside the body to draw cooling fluid and urine from the outlet passage.

8. An energy radiation applicator apparatus according to Claim 7, including a cooling fluid reservoir outside the body and in communication with the cooling fluid inlet passage, and wherein the cooling fluid reservoir is positioned to allow flow of fluid into the fluid receiving means to fill the fluid receiving means with cooling fluid.

9. An energy radiation applicator apparatus according to Claim 8, additionally including means for measuring the temperature of the cooling fluid entering the inlet passage, and means for measuring the temperature of the cooling fluid leaving the outlet passage, the difference in temperature being a function of the temperature of the tissue adjacent the fluid receiving means.

10. An energy radiation applicator apparatus according to Claim 9, including means for measuring the flow of cooling fluid through the fluid receiving means.

11. An energy radiation applicator apparatus according to Claim 1, additionally including means for measuring the temperature of cooling fluid prior to being

36

circulated through the fluid receiving means, and means for measuring the temperature of the cooling fluid after being circulated through the fluid receiving means, the difference in temperature being a function of the temperature of the tissue adjacent the fluid receiving means.

12. An energy radiation applicator apparatus according to Claim 11, including means for measuring the flow of cooling fluid through the fluid receiving means.

13. An energy radiation applicator apparatus according to Claim 1, wherein the means for connecting the applicator to a source of energy allows selective connection of the applicator to a source of energy to be supplied to the applicator, or to energy measurement means whereby energy can flow from the applicator to the energy measurement means.

14. An energy radiation applicator apparatus according to Claim 13, wherein the energy measurement means is a radiometer.

15. An energy radiation applicator apparatus for treatment of benign hyperplasia, comprising:

a catheter means for insertion into the urethra;

an applicator means attached to the catheter means, said applicator means including an applicator and a connector means extending through the catheter to outside the body;

energy measurement means; and

means for selectively coupling the connector means to either a source of energy sufficient to elevate the temperature of tissue surrounding the applicator to a preselected temperature and for maintaining the preselected temperature during treatment, or to the energy measurement means whereby energy received by the applicator from tissue surrounding the applicator is connected to the energy measurement means and is measured.
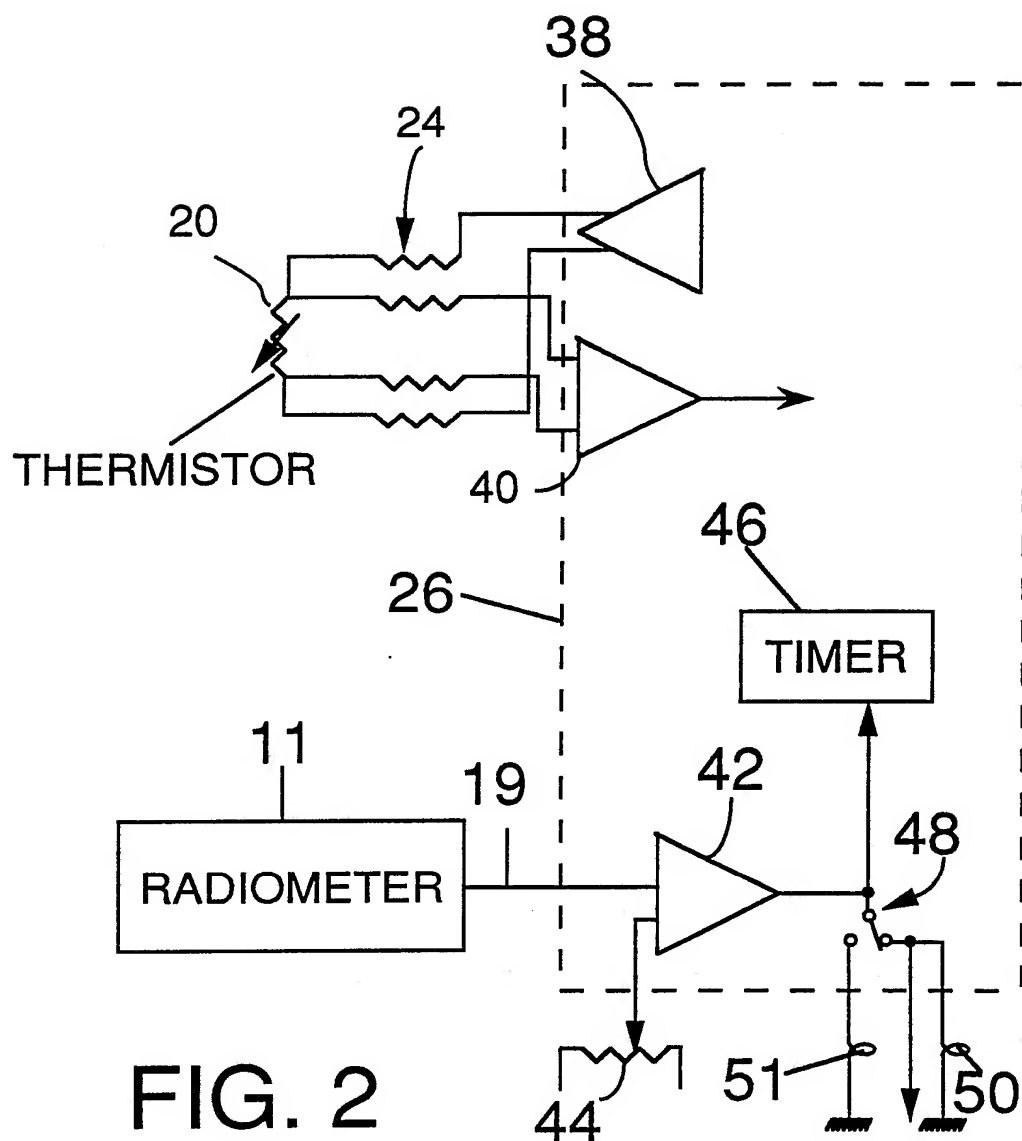
16. An energy radiation applicator apparatus according to Claim 15, wherein the energy measured by the

energy measurement means is indicative of the temperature
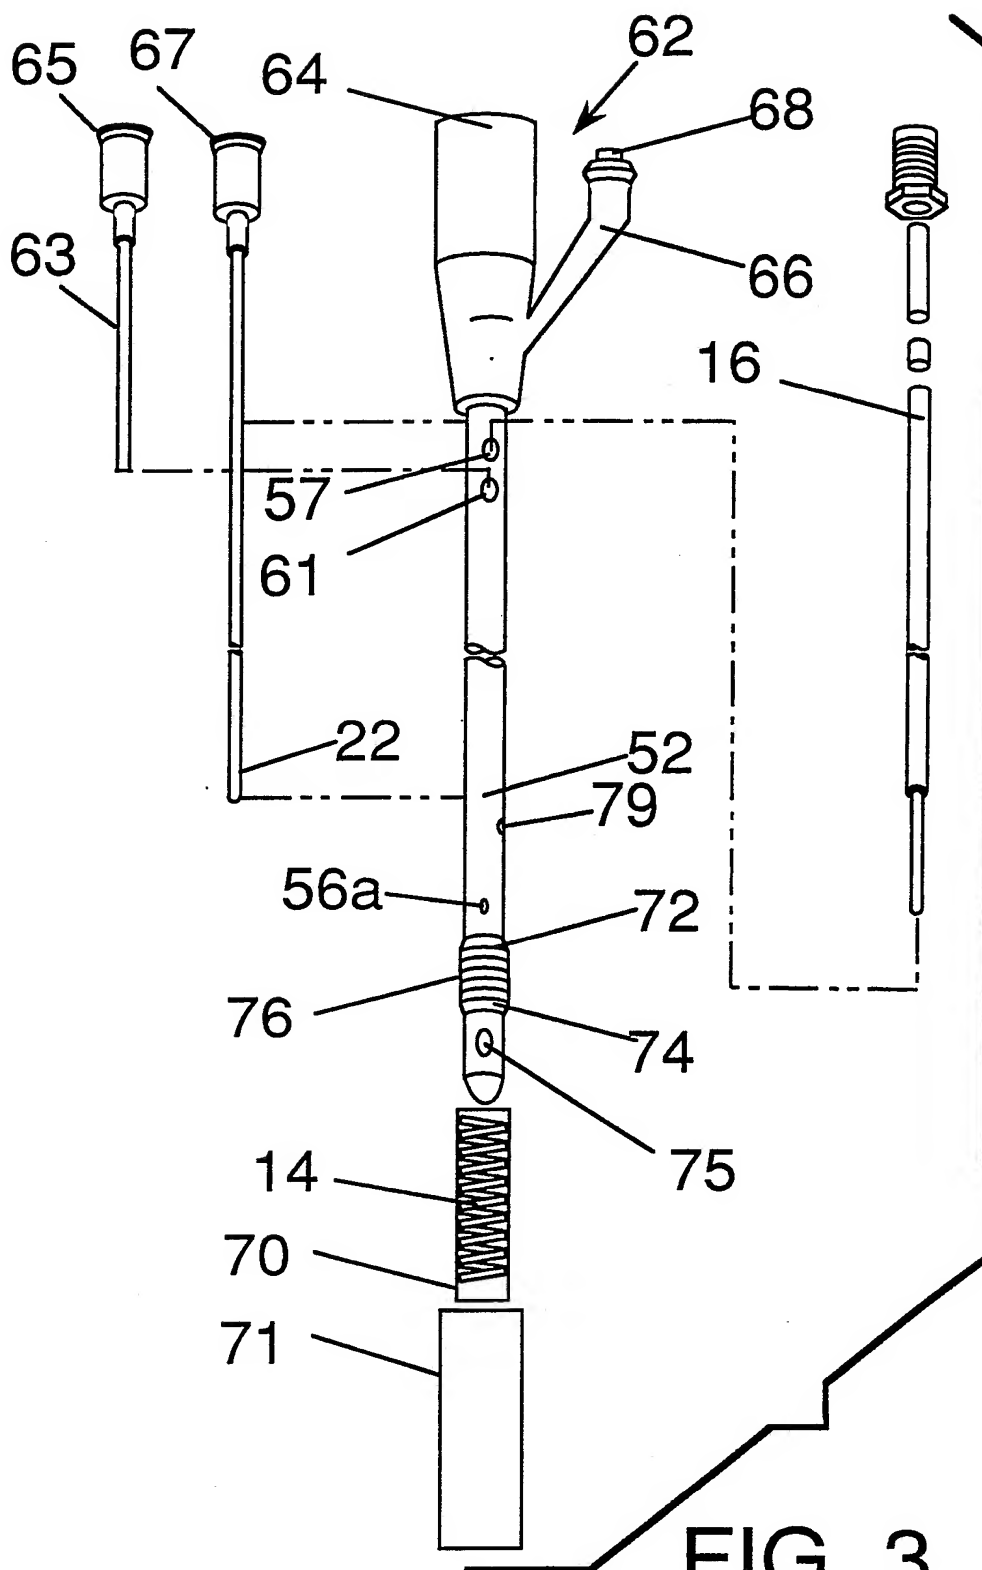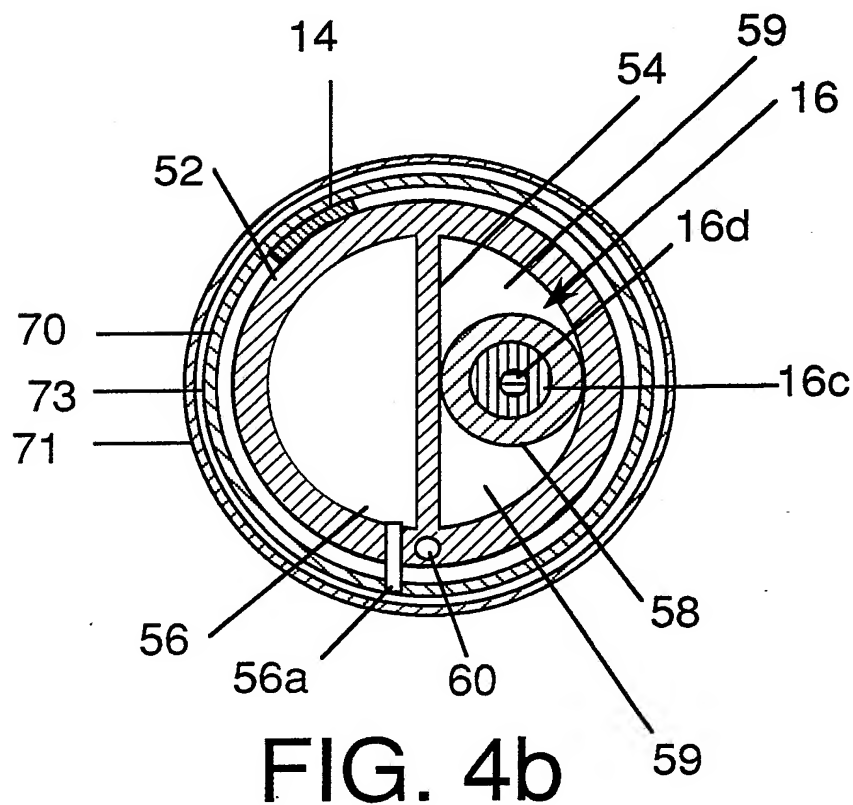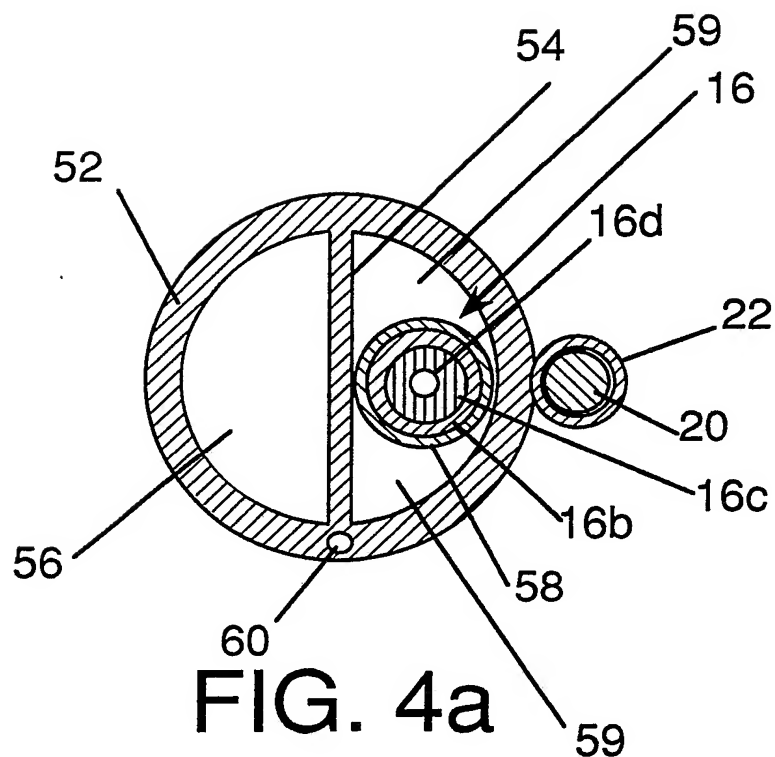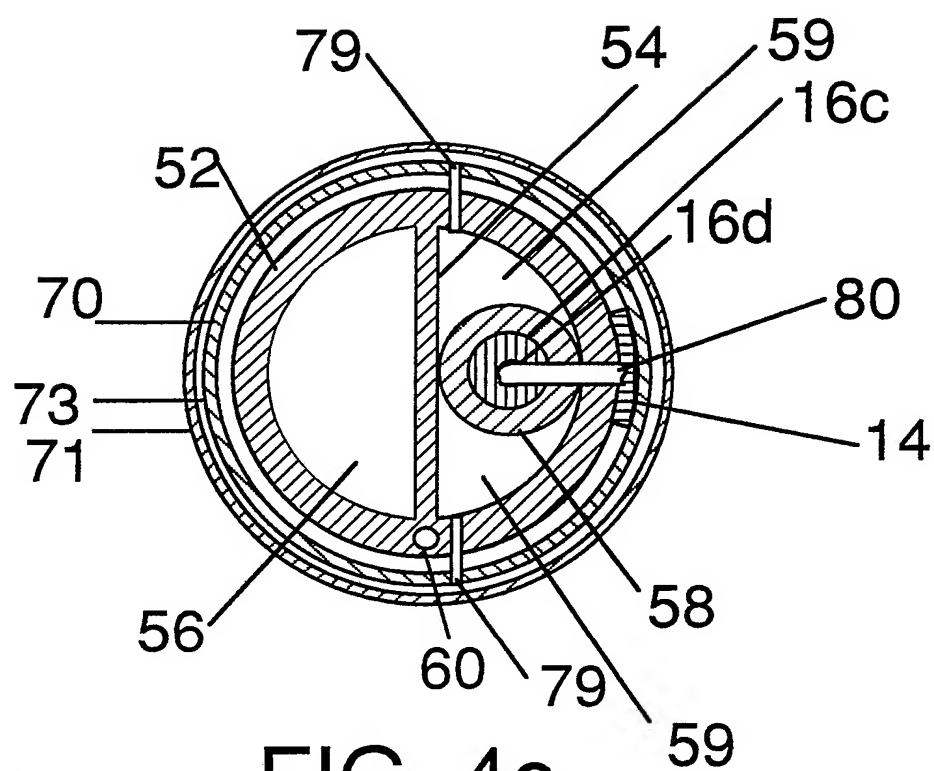of the tissue being heated by the applicator.

1/14

13 —— FILTER

MICROWAVE RADIOMETER — 11

16a   15   31 29   27

FILTER — 17

35
64

VACUUM PUMP

21   25 12

33

EM SOURCE

43

16

24

39

23

58   22

26

19

CONTROL CIRCUIT

28

10
52

CONTROL AND DISPLAY PANEL

ON   OFF

30   32   34   46a

4a   4a

FIG.1

4b   4b   18   20

4c   4c   37

14   76

CONDUCTIVE SHIELD

150

FIG. 2

FIG. 3

SUBSTITUTE SHEET

4/14

FIG. 4a

FIG. 4b

FIG. 4c

FIG. 5

FIG. 6

FIG. 7

13 — FILTER

ULTRASOUND
RADIOMETER — 11

31 29

16a 15 27

17

FILTER

35

64 16

VACUUM
PUMP

21 25 12

33

EM SOURCE
(US)

43

39

24

23

58 22

CONTROL
CIRCUIT

26 28 19

10
52

CONTROL AND
DISPLAY PANEL

ON   OFF

30   32   34   46a

FIG.8

18

20

14   37

76

FIG. 9

16d

16c

146

140

142

140

144

140

142

140

80

FIG. 10

FIG. 11

13/14

MICRO
PROCESSOR

160

158

27   FILTER   17

25 12

EM SOURCE

23

CONTROL
CIRCUIT

26   28   19

VACUUM
PUMP

35
64
33

16

39

MONITOR

154
156

152

10

52

43

24

22

58

CONTROL AND
DISPLAY PANEL

ON   OFF

30   32   34   46a

FIG.12

4a   4a

4b   4b   18   20

4c   4c   37

14   76

FIG. 13

INTERNATIONAL SEARCH REPORT

I. CLASSIFICATION OF SUBJECT MATTER (if several classification symbols apply, indicate all) 6

According to International Patent Classification (IPC) or to both National Classification and IPC

IPC(5): A61N 5/02
U.S. CL.: 128/786, 804, 401, 736

II. FIELDS SEARCHED

Minimum Documentation Searched 7

Classification System	Classification Symbols
U.S.	128/784-786,804,401,736

Documentation Searched other than Minimum Documentation to the Extent that such Documents are Included in the Fields Searched 8

III. DOCUMENTS CONSIDERED TO BE RELEVANT 9

Category *	Citation of Document, 11 with indication, where appropriate, of the relevant passages 12	Relevant to Claim No. 13
Y	US, A, 4,469,103 (BARRETT) 04 September 1984, See entire document.	9-12
A	US, A, 4,798,215 (TURNER) 17 January 1989, See entire document.	13-16
A	US, A, 4,813,429 (ESHEL) 21 March 1989, See entire document.	5
X,P / Y	US, A, 5,007,437 (STERZER) 16 April 1991, See entire document.	1-3 / 4-16
X / Y	EP, A, 0,370,890 (HASCOET) 30 May 1990, See entire document.	1-3 / 4-16
Y	DE, A, 2,815,156 (CONVERT) 19 October 1978, See entire document.	13-16
Y	SU, A, 1,512,622 (BDOC) 07 October 1989, See entire document.	5
A	EP, A, 0,105,677 (SOGAWA) 18 April 1984, See entire document.	1-12

* Special categories of cited documents: 10

"A" document defining the general state of the art which is not considered to be of particular relevance

"E" earlier document but published on or after the international filing date

"L" document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)

"O" document referring to an oral disclosure, use, exhibition or other means

"P" document published prior to the international filing date but later than the priority date claimed

"T" later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention

"X" document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step

"Y" document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art.

"&" document member of the same patent family

IV. CERTIFICATION

Date of the Actual Completion of the International Search	Date of Mailing of this International Search Report
28 JANUARY 1992	28 FEB 1992
International Searching Authority	Signature of Authorized Officer
ISA/US	LEE S. COHEN

Form PCT/ISA/210 (second sheet) (Rev.11-87)